


THE INFORMATION CONTAINED IN THIS DRAWING IS THE SOLE PROPERTY OF ALTIMATE MEDICAL. ANY REPRODUCTION IN PART OR WHOLE WITHOUT THE WRITTEN PERMISSION OF ALTIMATE MEDICAL IS PROHIBITED.

REVISIONS				
REV:	DESCRIPTION:	ECO #:	DATE:	APPROVED:
000	NEW RELEASE.	05-ECO-001	8/23/05	GJR
A	REVISED NG10344 TO REV A, ALSO ADD (2) M6 NUTS #600008	DCR-00730	11/11/10	JVS

NOTES:
 1. SLIP OVER HEAD REST BRACKET AFTER ASSEMBLY.
 2. REMOVE FLANGED NUT AND DISCARD BEFORE ASSEMBLY.

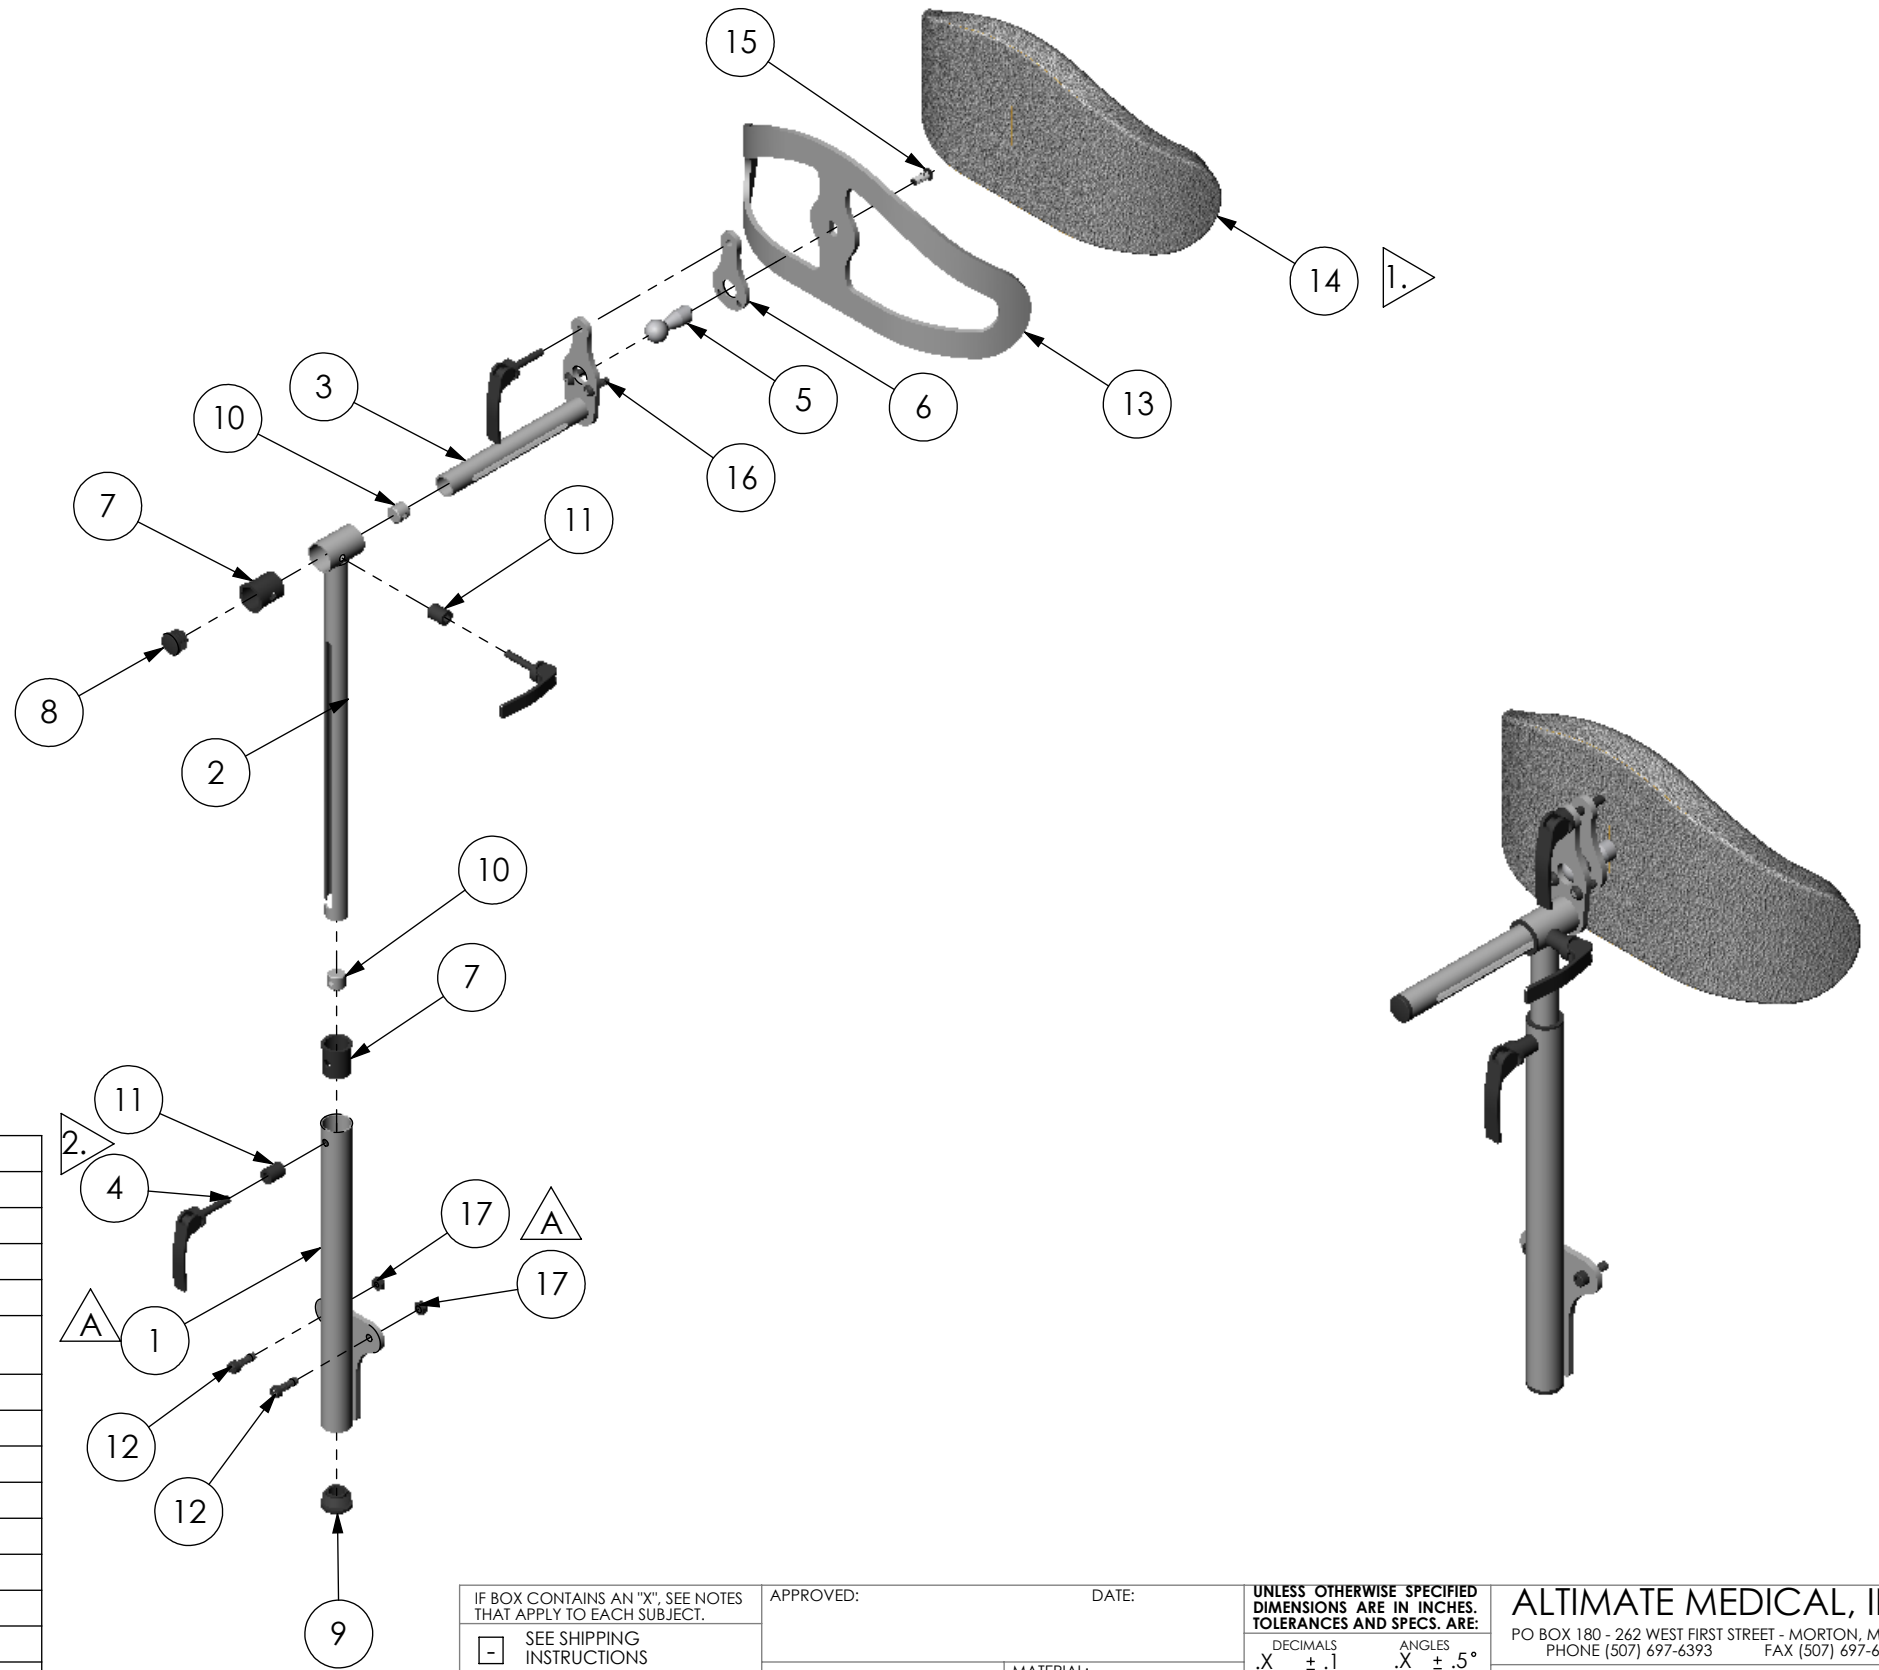

ITEM NO.	PART NO.	REV	QTY.	NAME
1	NG10344	A	1	BRACKET MOUNT HEAD REST
2	NG10347	B	1	BRACKET HEAD REST
3	NG10350	A	1	BRACKET HEAD REST
4	600017	000	3	CLAMP TOGGLE LOCK
5	80876	000	1	HEADREST BALL ATTACHMENT WHITMEYER
6	NG10353	000	1	TAB HEAD REST
7	NG20056	000	2	BUSHING HEAD REST
8	10071	-	1	.75 RND CAP
9	10073	-	1	CAP
10	600172	A	2	LUG HEAD REST ADJ.
11	80421	-	2	TABLE EXTENSION
12	600022	000	2	SHCS M6 X 1.0-20
13	NG10226	000	1	BRACEKT HEAD REST PLATE
14	NG30018	000	1	PAD HEAD REST LG
15	80757	-	1	BOLT 1/4-20 X 5/8 BTN SHCS
16	600029	-	2	BOLT BTN HD M6X1.-20
17	600008	000	2	NUT M6 X 1.0 NYLON LOCK

IF BOX CONTAINS AN "X", SEE NOTES THAT APPLY TO EACH SUBJECT. <input type="checkbox"/> SEE SHIPPING INSTRUCTIONS <input type="checkbox"/> RECIEVING INSPECTION <input type="checkbox"/> SEE ENVIRONMENTAL INSTRUCTIONS	APPROVED:	DATE:	UNLESS OTHERWISE SPECIFIED DIMENSIONS ARE IN INCHES. TOLERANCES AND SPECS. ARE: DECIMALS: .X ± .1 .XX ± .03 .XXX ± .015 ANGLES: .X ± .5° HOLE SIZE TOLERANCE: (+.005/- .000) BREAK EDGES .005 - .015 CMFR DRILLED HOLES .03 X 45°	ALTIMATE MEDICAL, INC. PO BOX 180 - 262 WEST FIRST STREET - MORTON, MN 56270 PHONE (507) 697-6393 FAX (507) 697-6900 DESCRIPTION: HEAD REST ASSEMBLY LG (V915) SIZE DWG. NO. NG50037 REV. A SCALE = 1:6 CAD FILE NAME: NG50037 SHEET 1 OF 1	
	DRAWN: MWL	DATE: 7/27/05			MATERIAL:
	OPTION NUMBER:	FINISH: -			CODE: ASMBLY